


Fig. 1








Fig.3



PRIOR ART

Fig. 4










Fig.5 PRIOR ART

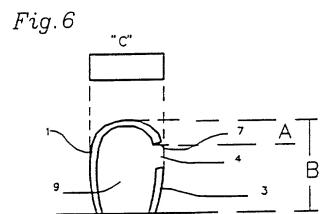



PRIOR ART

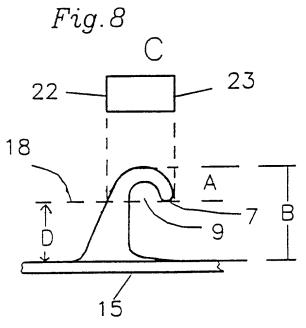





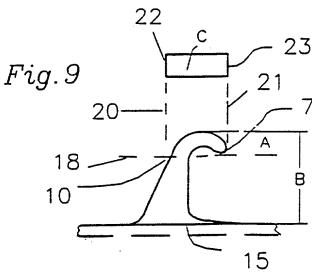



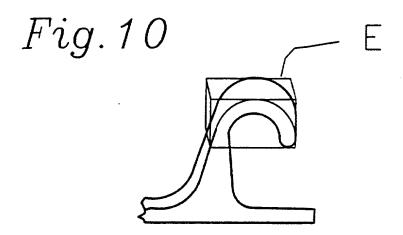

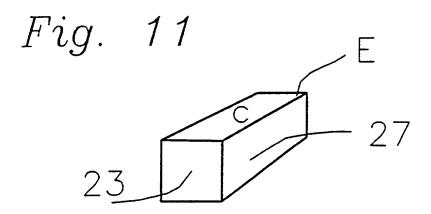

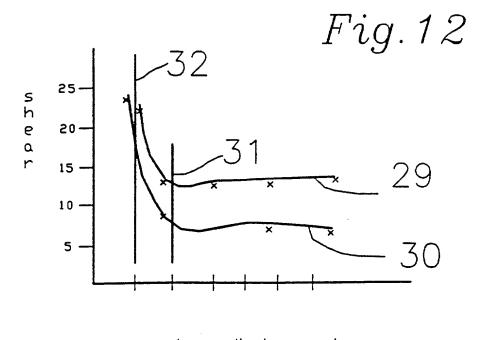

volume displacement

United States Patent & Trademark Office

Office of Initial Patent Examination -- Scanning Division



Application deficiencies found during scanning:

1.	Application papers are not suitable for scanning and are not in compliance with 37 CFR
	 1.52 because: ☐ All sheets must be the same size and either A4 (21 cm x 29.7 cm) or 8-1/2"x 11". Pages
2.	Drawings are not in compliance and were not scanned because: ☐ The drawings or copy of drawings are not suitable for electronic reproduction. ☐ All drawings sheets are not the same size. Pages must be either A4 (21 cm x 29.7 cm) or 8-1/2" x 11". ☐ Each sheet must include a top and left margin of at least 2.5 cm (1"), a right margin of at least 1.5 cm (9/16") and a bottom margin of at least 1.0 cm (3/8").
3.	Page(s) are not of sufficient clarity, contrast and quality for electronic reproduction.
4.	Page(s) are missing.
5.	OTHER: update